


# FeLV Virus Antigen One-Step

For the detection of viral p27 antigen in serum or plasma samples of cats and other felids (e.g. cheetah, lion)



24

January 2022

3

Please use only the valid version of the package insert provided with the kit.

# 1. Table of Contents

1.	Table of Contents	2
2.	Introduction	3
3.	Intended use of the test kit	3
4.	Principle of the test kit	4
5.	Contents	4
6.	Handling and storage of specimens	4
7.	Sample material	4
8.	Precautions	4
9.	Test protocol	5
10.	Validation of the test	5
11.	Interpretation of the test results	6
12.	Symbols used with EVL ASSAYS	7

# 2. Introduction


FeLV is a retrovirus (oncogenic RNA virus) which causes persistent infection of domestic cats and other felids. Persistently infected cats shed the virus and invariably develop fatal diseases including Leukemia, Lymphosarcoma, Anaemia, Immuno-deficiency and Enteritis. Most cases of disease are found in cats aged 2-4 years old.

FeLV is shed in all body secretions (saliva/urine/tears/milk/faeces), but the virus is transmitted mainly by biting, mating, through the milk and in utero. Kittens under 3 months are very susceptible to infection, however susceptibility declines after 4 months of age. During the incubation period between infection and development of disease, persistently infected cats are healthy but are viraemic and therefore a source of infection for other cats. In Europe, approximately 1-5% of healthy cats are FeLV positive. With sick cats this proportion rises to around 20%.

The blood of FeLV infected cats contain high levels of FeLV p27, the major core protein of the virus (see diagram). The FeLV One-Step test rapidly and specifically detects the p27 antigen in the serum or plasma.

For this reason, the test is suitable for the detection of viraemic cats, both for the confirmation of diagnosis of disease and for the prevention of the spread of FeLV infection in households of cats.

Diagram FeLV:

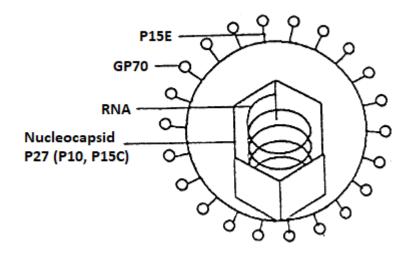

# 3. Intended use of the test kit

This One-Step test is intended to use as practical/routine screening test that can be done in a few minutes. This test kit is designed to detect FeLV p27 antigen by use of a Rapid Immunochromatic Assay.

BV European Veterinary Laboratory Postbus 198 3440 AD Woerden The Netherlands m

# 4. Principle of the test kit

The FeLV One-Step test is based on a chromatographic test strip, a monoclonal antibody and a polyclonal antibody which react with different epitopes of the FeLV p27 antigen. The polyclonal antibodies are conjugated to colloidal gold particles and the monoclonal antibody is immobilized on the strip in the test zone "T". FeLV p27 antigen in a sample that is applied to the strip at the sample zone "S" will bind to the gold particles which then migrate to zone "T". A colour change in zone "T" indicates a positive test.

Labelled colloidal gold particles are also immobilized on the test strip in the control zone "C", to indicate that the test is working properly.

## 5. Contents

- 24 x Pouches, each containing 1 test strip and 1 pipette
- 1 x Dropper bottle
- 1 x Protocol

# 6. Handling and storage of specimens

The One-Step should be stored at room temperature ( $\pm 21^{\circ}$ C). An unopened package can be used until the expiry date. An opened package must be used immediately. If the conditions are no longer fulfilled the test can no longer be used. Avoid freezing and heating as this will contribute to destruction of the test. Samples may be used fresh or may be kept frozen below -20°C before use.

## 7. Sample material

It is advised to test fresh serum or plasma samples. Do not use haemolytic or lipemic serum.


## 8. Precautions

- Handle all biological materials as though capable of transmitting infectious diseases.
- Do not pipette by mouth
- Do not eat, drink, smoke, prepare foods or apply cosmetics within the designated work area.
- Do not use components which passed the expiry date and do not mix components from different serials lots together.
- Optimal results will be obtained by strict adherence to this protocol. Careful pipetting and sampling throughout this procedure are necessary to maintain precision and accuracy.
- Each test strip is ultimately used as an optical reference. Therefore, do not touch the surface of the test strip and protect it from damage and dirt.

BV European Veterinary Laboratory Postbus 198 3440 AD Woerden The Netherlands Tel: +31 (0)348-412549 Web: www.evlonline.org @: info@evlonline.eu 4

# 9. Test protocol

- 1. Unpack the test strip, swab and pipette. Only open the amount of pouches to be used. An opened package should be used immediately.
- 2. Add **1 drop** of buffer from the dropper bottle to the sample zone (Figure 1).
- 3. Add **2 drops** of the sample to the sample zone by using the pipette (Figure 2).
- 4. Add **1 drop** of buffer from the dropper bottle to the sample zone (Figure 3).
- 5. Read the result after 5-20 minutes (for the interpretation of the test result see chapter 10 and chapter 11).

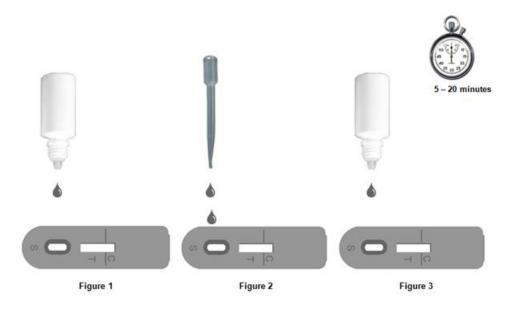

# **10.** Validation of the test

To validate an EVL One-Step a control line should always be visible at control zone "C". If no control line is visible the test should be considered invalid.

Results should be read in the given time. Results read after the given time should be considered invalid. Invalid tests should be repeated with a new test.

# **11.** Interpretation of the test results

### Positive:

Two lines are visible in zone "T" and in zone "C" (Figure A). The sample contains FeLV p27. Positive results may vary in optical density due to variations in viral concentrations in the sample.

#### Weak positive:

Two lines are visible, a weak line in zone "T" and a line in zone "C" (Figure B). The sample contains low concentrations of FeLV p27 antigen.

#### Negative:

Only one line is visible in zone "C" (Figure C). The sample does not contain FeLV p27 antigen.

#### Not valid:

No line is visible in zone "C" (fig. D). Repeat the test procedure with a new test cassette.







Figure A: Positive

Figure B: Weak positive

Figure C: Negative




Figure D: Not Valid **12.** Symbols used with EVL ASSAYS

<u>Symbol</u>	English
Ĩ	Consult instructions for use
CE	European Conformity
IVD	In vitro diagnostic device
RUO	For research use only
REF	Catalogue number
LOT	Lot/ No. / Batch code
Σ	Contains sufficient for <n> tests</n>
	Storage Temperature
	Expiration Date
	Legal Manufacturer
Distributed by	Distributor
Content	Content
Volume/No.	Volume / No.

The entire risk as to the performance of these products is assumed by the purchaser. EVL shall not be liable for indirect, special or consequential damages of any kind resulting from use of the products. In case of problems or questions contact EVL.

BV European Veterinary Laboratory Postbus 198 3440 AD Woerden The Netherlands Tel: +31 (0)348-412549 Web: www.evlonline.org @: info@evlonline.eu